

GASTEC No.1A Instructions for Carbon Monoxide Airtec Tube

FOR SAFE OPERATION :

Carefully read this manual.

⚠ CAUTION : If you do not observe the following precautions, you may suffer injuries or damage to the product.

1. When breaking the tube ends, keep away from eyes.
2. Do not touch the broken glass tubes, pieces and reagent with bare hand(s).

⚠ NOTES : For maintaining performance and reliability of the test results, observe the following.


1. Use this tube within the temperature range of 0 - 40°C (32 - 104°F).
2. Use this tube within the relative humidity range of 0 - 90%.
3. Shelf life and storage condition of the tube are marked on the label of the box of tube.

APPLICATION OF THE TUBE :

Use this tube for the detection of Carbon monoxide, simply connect the pressure reducer to your high pressure air source, compressor, cylinder, or air line and adjust the flow metre to the required setting.

SPECIFICATION :

(Because of Gastec's commitment to continued improvement, specifications are subject to change without notice.)



Measuring Range	5 – 50 ppm
Sampling Volume (Flow Metre)	300 mL
Sampling Rate	100 mL/min
Sampling Time	3 minutes
Colour Change	Yellow → Blackish brown
Reaction Principle	$\text{CO} + \text{Na}_2\text{Pd}(\text{SO}_3)_2 \rightarrow \text{Pd} + \text{CO}_2 + \text{SO}_2 + \text{Na}_2\text{SO}_3$

Coefficient of Variation: 10% (for 5 to 10 ppm), 5% (for 10 to 50 ppm)

**** Shelf Life: Please refer to the validity date printed on the box of tube.**

**** Store the tubes in the cool and dark place.**

CORRECTION FOR TEMPERATURE, HUMIDITY AND PRESSURE :

Temperature : No correction is required.


Humidity : No correction is required.

Pressure : To correct for pressure, multiply the tube reading by


$$\frac{\text{Tube Reading (ppm)} \times 1013 \text{ (hPa)}}{\text{Atmospheric Pressure (hPa)}}$$

MEASUREMENT PROCEDURE :


1. Attach a pressure reducer with gauge and flow metre to a cylinder, compressor or air line and adjust the flow metre to the required setting.
2. Break the tips off a fresh detector tube using the tube tip breaker and insert the tube into a tube holder.

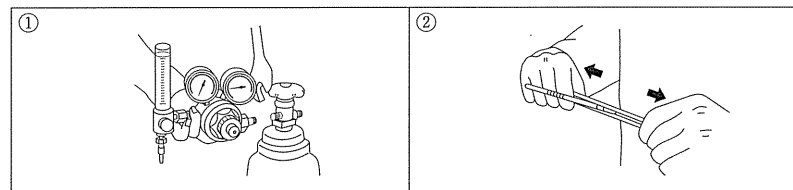

3. Attach the rubber tube holder to the flow metre outlet. Make sure the tube arrow (➔) on the tube is pointing in the downward direction.
4. Turn on the cylinder or compressor and confirm the flow metre according to each Airtec tube specifications.

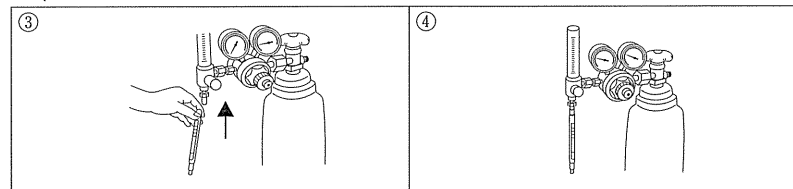

5. Time the sampling with a stopwatch.
6. As soon as the sampling time has finished, turn off the cylinder or compressor, and remove the tube from the tube holder and then read the colour-changed layer immediately.

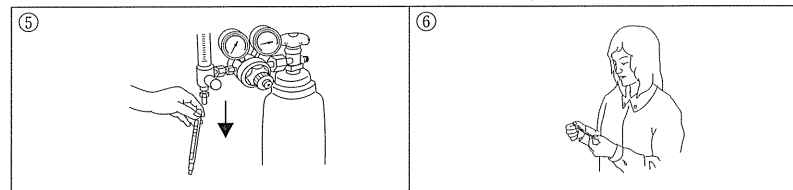

7. If the sampling volume deviates from the volume specified in this instruction manual, correct the tube reading by the following formula. In this case, use the concentration as a reference.

$$\text{Concentration (ppm)} = \frac{\text{Tube Reading} \times 300}{\text{Sampled Volume (mL)}}$$

Use of the Compressed Breathing Air Measurement Kit Model. No.CG-1

When Airtec tube used with the Model. No. CG-1 kit, make sure to preset the flow rate of the CG-1 device and adjust the sampling time according to the following table. For the measurement procedure, carefully read and follow the instruction manual supplied with the CG-1 kit.

Measuring Range	5 – 50 ppm
Sampling Time	5 minutes
Specified Flow Rate	100 mL/min(±10 mL/min)
Correction Factor	1
Colour Change	Yellow → Blackish brown
Reaction Principle	$\text{CO} + \text{Na}_2\text{Pd}(\text{SO}_3)_2 \rightarrow \text{Pd} + \text{CO}_2 + \text{SO}_2 + \text{Na}_2\text{SO}_3$

DANGEROUS AND HAZARDOUS PROPERTIES :

Threshold Limit Value-Time Weighted Average by ACGIH (2016): 25 ppm

Explosive Range: 12.5 – 74%

INSTRUCTIONS ON DISPOSAL :

The reagent of the tube does not use toxic substances. When disposing the tube regardless of whether it has been used or unused, follow the rules and regulations of your local government.

WARRANTY :

If you have any questions regarding gas detection and quality of the tubes, please feel free to contact your Gastec representatives.

Manufacturer : Gastec Corporation
8-8-6 Fukayanaka, Ayase-City, Kanagawa 252-1195, Japan
<http://www.gastec.co.jp/>
Telephone +81-467-79-3910 Facsimile +81-467-79-3979

IM011AE2
Printed in Japan
17E1Z